

Avian Influenza Virus Antigen Rapid Test Kit

Catalog No.: abx092015

Size: 40 tests

Storage: Store all reagents at 2-30 °C. Keep dry.

Application: For qualitative detection of Avian Influenza Virus Antigen in poultry excrement or laryngotracheal secretions.

Introduction and assay principle

Abbexa's Avian Influenza Virus Antigen Rapid Test Kit is a qualitative lateral flow immunochromatographic assay for the detection of Avian Influenza Virus (AIV) Antigen in poultry samples. The cassette contains a colloidal gold conjugated antibody against AIV, which combines with any AIV antigen present in the samples. The complex binds with the antibody coated on the test region of the cassette. A colored band develops within 15 minutes in the test region if the concentration of AIV antigen in the sample is higher than the detection limit. A control region on the upper end of the cassette confirms if the test has been successful.

Kit Components

- Test cassettes with pipettes: 40
- Sample diluent: 40 vials
- Cotton swabs: 40

Material Required But Not Provided

- Timer

Sample preparation

1. Using a cotton swab, take 0.1 g or 100 µl of poultry excrement or laryngotracheal secretion. Ensure that sufficient sample has been collected on the swab. **Note:** Do not use excessive quantities of stool samples as this may lead to black bands forming in the test result window, which will cause an invalid result.
2. Immediately insert the cotton swab into a tube containing Sample Diluent. Stir until the sample has completely dissolved. Wipe the swab against the inside of the tube, then discard the swab. Allow the mixture to stand at room temperature for 1-2 min.

Assay procedure


1. Take a test cassette and lay it flat on a clean table. Using the provided pipette, add 5 drops of prepared sample to the sample well on the test cassette. Avoid touching the membrane in the middle of the sample well, and avoid foaming.
2. Leave at room temperature for 10-15 min, then analyze the result.

Instructions for Use

Version: 1.1.1
Revision date: 27-Mar-24

Results analysis

- **Positive result:** A line is observed in both the control (C) section and the test (T) section.
- **Negative result:** A line is observed in the control (C) section but not the test (T) section.
- **Invalid result:** No line is observed in the control (C) section.

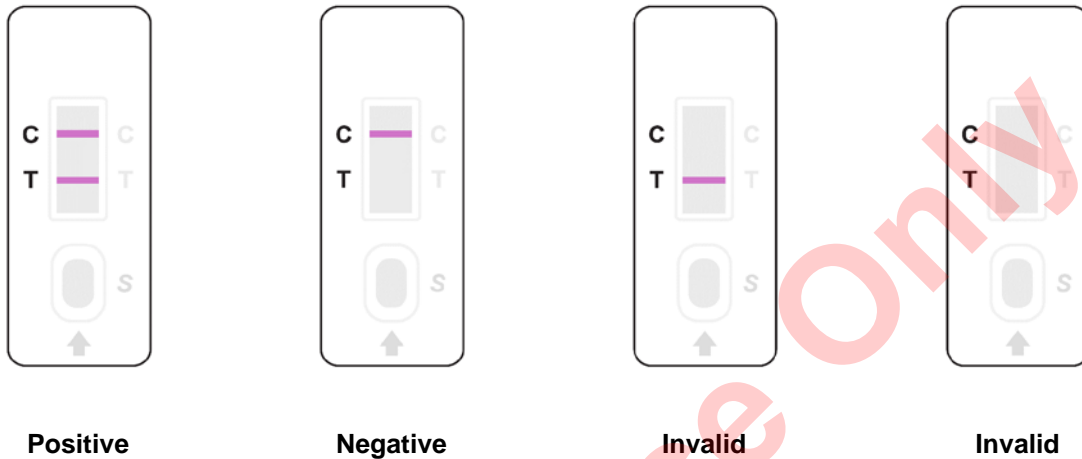

Notes

1. The test cassettes should be brought to room temperature before use.
2. After opening the aluminum foil, use the test cassette as soon as possible.
3. Samples should be clear with no visible particles, turbidity, or bacterial pollution.
4. Do not mix or re-use the disposable pipettes to avoid cross-contamination.
5. Do not use water or PBS as the negative control.
6. Avoid touching the cassette membrane through the sample well or test result window.
7. This kit is for qualitative detection of AIV antigen in poultry samples. It cannot distinguish between the different AIV subtypes.
8. This kit is for research use only and the results are for reference only. It is recommended to use this kit in conjunction with another detection method.
9. All waste should be disposed of appropriately. Please note that you may need to follow special waste disposal procedures for infectious samples. Please check local disposal regulations.